

# **EMC TEST REPORT**

**For**

**Shenzhen New Huayi Instrument Co., Ltd**

**Temperature Humidity Meter**

**Model No.: MS6508**

**Prepared for : Shenzhen New Huayi Instrument Co., Ltd**  
**Address : F3, Block 2, Instrument World Industrial Park, Guiyue Road, Longhua New District, Shenzhen City**

**Prepared by : LiTest Technology Service Co., Ltd.**  
**Address : No.42 FuKang Road, HouJie Town DongGuan City, GuangDong Province, China**

**Tel: +86-769-82272566**  
**Fax: +86-769-82272565**  
**Email:service@litest.cn**

**Report No. : 16LTE030929E**  
**Date of Test : March 9-18, 2016**  
**Date of Report : March 21, 2016**

## Table of Contents

| Description  | Page |
|--|------|
| TEST REPORT VERIFICATION .....   | 6    |
| 1 SUMMARY OF TEST RESULTS .....  | 7    |
| 1.1 DESCRIPTION OF STANDARDS AND RESULTS .....                                 | 7    |
| 2 GENERAL INFORMATION .....  | 8    |
| 2.1 Description of Device (EUT) .....  | 8    |
| 2.2 Tested Supporting System Details .....                                     | 9    |
| 2.3 Block Diagram of connection between EUT and simulators .....               | 9    |
| 2.4 Test Facility .....  | 10   |
| 2.4.1 Laboratory Name: .....   | 10   |
| 2.4.2 Site Location .....  | 10   |
| 2.4.3 Test facility: .....   | 10   |
| 2.5 Measurement Uncertainty .....  | 10   |
| 2.6 Test Mode Description .....  | 10   |
| 3 CONDUCTED DISTURBANCE AT MAINS TERMINALS TEST .....                          | 11   |
| 3.1 Test Equipment .....   | 11   |
| 3.2 Block Diagram of Test Setup .....  | 11   |
| 3.3 Test Standard .....  | 11   |
| 3.4 Power Line Conducted Disturbance at Mains Terminals Limit .....            | 11   |
| 3.5 EUT Configuration on Test .....  | 12   |
| 3.5.1 Support Equipment : .....  | 12   |
| 3.6 Operating Condition of EUT .....   | 12   |
| 3.6.1 Setup the EUT and simulator as shown as Section 3.2. ....                | 12   |
| 3.6.2 Turn on the power of all equipment .....                                 | 12   |
| 3.6.3 Let EUT work in test modes and measure it. ....                          | 12   |
| 3.7 Test Procedure .....   | 12   |
| 3.8 Conducted Disturbance At Mains Terminals Test Results .....                | 12   |
| 4 RADIATED DISTURBANCE TEST .....  | 13   |
| 4.1 Test Equipments .....  | 13   |
| 4.1.1 For Frequency Range 30MHz~1000 MHz (At Semi Anechoic Chamber) .....      | 13   |
| 4.1.2 For Frequency Range 1GHz~6 GHz (At Semi Anechoic Chamber) .....          | 13   |
| 4.2 Block Diagram Of Test Setup .....  | 13   |
| 4.2.1 In Semi Anechoic Chamber (3m) Test Setup Diagram For 30MHz~1000MHz ..... | 13   |
| 4.2.2 In Semi Anechoic Chamber (3m) Test Setup Diagram for 1-6GHz .....        | 14   |
| 4.3 Test Standard .....  | 14   |
| 4.4 Radiated Disturbance Limit .....   | 14   |
| 4.5 EUT Configuration on Test .....  | 15   |
| 4.6 Operating Condition of EUT .....   | 15   |
| 4.6.1 Setup the EUT and simulator as shown as Section 4.2. ....                | 15   |
| 4.6.2 Turned on the power of all equipment .....                               | 15   |
| 4.6.3 Let EUT work in test modes and measure it. ....                          | 15   |
| 4.7 Test Procedure .....   | 15   |
| 4.8 Radiated Disturbance Test Results .....                                    | 16   |
| 5 HARMONIC CURRENT TEST .....  | 19   |
| 5.1 Test Equipments .....  | 19   |

|       |   |    |
|-------|---|----|
| 5.2   | Block Diagram of Test Setup .....                       | 19 |
| 5.3   | Test Standard .....                                     | 19 |
| 5.4   | Limits of Harmonic Current .....                        | 19 |
| 5.5   | Operating Condition of EUT .....                        | 20 |
| 5.6   | Test Procedure .....                                    | 21 |
| 5.7   | Test Results .....                                      | 21 |
| 6     | VOLTAGE FLUCTUATIONS & FLICKER TEST .....               | 22 |
| 6.1   | Test Equipment .....                                    | 22 |
| 6.2   | Block Diagram of Test Setup .....                       | 22 |
| 6.3   | Test Standard .....                                     | 22 |
| 6.4   | Limits of Voltage Fluctuation and Flick .....           | 22 |
| 6.5   | Operating Condition of EUT .....                        | 22 |
| 6.6   | Test Procedure .....                                    | 22 |
| 6.7   | Test Results .....                                      | 22 |
| 7     | IMMUNITY PERFORMANCE CRITERIA .....                     | 23 |
| 8     | ELECTROSTATIC DISCHARGE IMMUNITY TEST .....             | 24 |
| 8.1   | Test Equipments .....                                   | 24 |
| 8.2   | Block Diagram of Test Setup .....                       | 24 |
| 8.3   | Test Standard .....                                     | 24 |
| 8.4   | Severity Levels and Performance Criterion .....         | 24 |
| 8.4.1 | Severity level .....                                    | 24 |
| 8.4.2 | Performance criterion : B .....                         | 24 |
| 8.5   | EUT Configuration .....                                 | 25 |
| 8.6   | Operating Condition of EUT .....                        | 25 |
| 8.7   | Test Procedure .....                                    | 25 |
| 8.7.1 | Air Discharge: .....                                    | 25 |
| 8.7.2 | Contact Discharge: .....                                | 25 |
| 8.7.3 | Indirect discharge for horizontal coupling plane: ..... | 25 |
| 8.7.4 | Indirect discharge for vertical coupling plane: .....   | 25 |
| 8.8   | Test Results .....                                      | 25 |
| 9     | RF FIELD STRENGTH SUSCEPTIBILITY TEST .....             | 27 |
| 9.1   | Test Equipments .....                                   | 27 |
| 9.2   | Block Diagram of Test Setup .....                       | 27 |
| 9.3   | Test Standard .....                                     | 28 |
| 9.4   | Severity Levels and Performance Criterion .....         | 28 |
| 9.4.1 | Limit .....   | 28 |
| 9.4.2 | Severity level .....                                    | 28 |
| 9.4.3 | Performance criterion : A .....                         | 28 |
| 9.5   | EUT Configuration .....                                 | 28 |
| 9.6   | Operating Condition of EUT .....                        | 28 |
| 9.7   | Test Procedure .....                                    | 29 |
| 9.8   | Test Results .....                                      | 29 |
| 10    | ELECTRICAL FAST TRANSIENT/BURST IMMUNITY TEST .....     | 33 |
| 10.1  | Test Equipments .....                                   | 33 |
| 10.2  | Block Diagram of Test Setup .....                       | 33 |
| 10.3  | Test Standard .....                                     | 33 |
| 10.4  | Severity Levels and Performance Criterion .....         | 33 |

|        |  |    |
|--------|--|----|
| 10.4.1 | Severity level .....                           | 33 |
| 10.4.2 | Performance criterion : B .....                | 33 |
| 10.5   | EUT Configuration .....                        | 34 |
| 10.6   | Operating Condition of EUT .....               | 34 |
| 10.7   | Test Procedure .....                           | 34 |
| 10.7.1 | For input and AC power ports: .....            | 34 |
| 10.7.2 | For signal lines and control lines ports:..... | 34 |
| 10.7.3 | For DC input and DC output power ports:.....   | 34 |
| 10.8   | Test Results.....                              | 34 |
| 11     | SURGE TEST .....                               | 35 |
| 11.1   | Test Equipments.....                           | 35 |
| 11.2   | Block Diagram of Test Setup .....              | 35 |
| 11.3   | Test Standard .....                            | 35 |
| 11.4   | Severity Levels and Performance Criterion..... | 35 |
| 11.4.1 | Severity level .....                           | 35 |
| 11.4.2 | Performance criterion: B .....                 | 35 |
| 11.5   | EUT Configuration .....                        | 36 |
| 11.6   | Operating Condition of EUT .....               | 36 |
| 11.7   | Test Procedure .....                           | 36 |
| 11.8   | Test Results.....                              | 36 |
| 12     | INJECTED CURRENTS SUSCEPTIBILITY TEST.....     | 37 |
| 12.1   | Test Equipments.....                           | 37 |
| 12.2   | Block Diagram of Test Setup .....              | 37 |
| 12.3   | Test Standard .....                            | 37 |
| 12.4   | Severity Levels and Performance Criterion..... | 37 |
| 12.4.1 | Severity level .....                           | 37 |
| 12.4.2 | Performance criterion: A .....                 | 37 |
| 12.5   | EUT Configuration .....                        | 38 |
| 12.6   | Operating Condition of EUT.....                | 38 |
| 12.7   | Test Procedure .....                           | 38 |
| 12.8   | Test Results.....                              | 38 |
| 13     | MAGNETIC FIELD IMMUNITY TEST .....             | 39 |
| 13.1   | Test Equipments.....                           | 39 |
| 13.2   | Block Diagram of Test Setup .....              | 39 |
| 13.3   | Test Standard .....                            | 39 |
| 13.4   | Severity Levels and Performance Criterion..... | 39 |
| 13.4.1 | Severity level .....                           | 39 |
| 13.4.2 | Performance criterion : A .....                | 39 |
| 13.5   | EUT Configuration on Test .....                | 40 |
| 13.6   | Operating Condition of EUT.....                | 40 |
| 13.7   | Test Procedure .....                           | 40 |
| 13.8   | Test Results.....                              | 40 |
| 14     | VOLTAGE DIPS AND INTERRUPTIONS TEST .....      | 42 |
| 14.1   | Test Equipment.....                            | 42 |
| 14.2   | Block Diagram of Test Setup .....              | 42 |
| 14.3   | Test Standard .....                            | 42 |
| 14.4   | Severity Levels and Performance Criterion..... | 42 |
| 14.4.1 | Severity level .....                           | 42 |

|        |  |    |
|--------|--|----|
| 14.4.2 | Performance criterion : B & C .....                          | 42 |
| 14.5   | EUT Configuration .....                                      | 43 |
| 14.6   | Operating Condition of EUT .....                             | 43 |
| 14.7   | Test Procedure .....   | 43 |
| 14.8   | Test Results .....   | 43 |
| 15     | PHOTOGRAPHS OF THE TEST CONFIGURATION .....                  | 44 |
| 15.1   | Photos of Radiated Emission Test (In Anechoic Chamber) ..... | 44 |
| 15.2   | Photos of Electrostatic Discharge Immunity Test.....         | 45 |
| 16     | PHOTOS OF THE EUT .....                                      | 46 |

**TEST REPORT VERIFICATION**

Applicant : Shenzhen New Huayi Instrument Co., Ltd

Manufacturer : Shenzhen New Huayi Instrument Co., Ltd

EUT Description : Temperature Humidity Meter

|                    |                    |
|--------------------|--------------------|
| (A) Model No :     | MS6508             |
| (B) Trademark :    | PEAKMETER          |
| (C) Power Supply:  | --                 |
| (D) Test Voltage : | DC 6V From Battery |

## Measurement Standard Used:

EN 61326-1: 2013

EN 61326-2-2: 2013

(IEC 61000-4-2:2008, IEC 61000-4-3:2006+A1:2007+A2:2010, IEC 61000-4-8:2009,)

The device described above is tested by LiTest Technology Service Co., Ltd.. to determine the maximum emission levels emanating from the device and the severe levels of the device can endure and its performance criterion. The test results are contained in this test report and LiTest Technology Service Co., Ltd. is assumed full responsibility for the accuracy and completeness of test. Also, this report shows that the EUT is technically compliant with the EN 61326-1 and EN 61326-2-2 requirements.

This report applies to above tested sample only.

Report of date..... : March 21, 2016

Tested by (name + signature).....:



Approved by (name + signature)..... :



## 1 SUMMARY OF TEST RESULTS

### 1.1 DESCRIPTION OF STANDARDS AND RESULTS

The EUT have been tested according to the applicable standards as referenced below

| EMISSION  |                                      |                      |                      |         |
|---|--------------------------------------|----------------------|----------------------|---------|
| Description of Test Item  | Standard                             | Limits               |                      | Results |
| Conducted disturbance at mains terminals  | EN 61326-1: 2013                     | Class B              |                      | N/A     |
| Conducted disturbance at telecommunication port   | EN 61326-1: 2013                     | Class B              |                      | N/A     |
| Radiated disturbance  | EN 61326-1: 2013                     | Class B              |                      | PASS    |
| Harmonic current emissions  | EN 61000-3-2:2014                    | Class A              |                      | N/A     |
| Voltage fluctuations & flicker  | EN 61000-3-3:2013                    | Section 5            |                      | N/A     |
| IMMUNITY (EN 61326-2-2: 2013)   |                                      |                      |                      |         |
| Description of Test Item  | Basic Standard                       | Performance Criteria | Observation Criteria | Results |
| Electrostatic discharge (ESD)   | IEC 61000-4-2:2008                   | B                    | B                    | PASS    |
| Radio-frequency, Continuous radiated disturbance  | IEC 61000-4-3:2006 +A1:2007+ A2:2010 | A                    | A                    | PASS    |
| Electrical fast transient (EFT)   | IEC 61000-4-4:2012                   | B                    | N/A                  | N/A     |
| Surge (Input a.c. power port)   | IEC 61000-4-5:2014                   | B                    | N/A                  | N/A     |
| Surge(Telecommunication port)   |                                      | B                    | N/A                  | N/A     |
| Radio-frequency, Continuous conducted disturbance   | IEC 61000-4-6:2013                   | A                    | N/A                  | N/A     |
| Power frequency magnetic field  | IEC 61000-4-8:2009                   | A                    | A                    | PASS    |
| Voltage dips, >95% reduction  | IEC 61000-4-11:2004                  | B                    | N/A                  | N/A     |
| Voltage dips, 30% reduction   |                                      | B                    | N/A                  | N/A     |
| Voltage interruptions   |                                      | C                    | N/A                  | N/A     |
| N/A is an abbreviation for Not Applicable.<br>The product intended for use in industrial locations. |                                      |                      |                      |         |

## 2 GENERAL INFORMATION

### 2.1 Description of Device (EUT)

|                    |   |                            |
|--------------------|---|----------------------------|
| <b>DESCRIPTION</b> | : | Temperature Humidity Meter |
|--------------------|---|----------------------------|

|                  |   |        |
|------------------|---|--------|
| <b>MODEL NO.</b> | : | MS6508 |
| <b>DIFF.</b>     | : | None   |

|                  |   |           |
|------------------|---|-----------|
| <b>TRADEMARK</b> | : | PEAKMETER |
|------------------|---|-----------|

|                  |   |   |
|------------------|---|---|
| <b>APPLICANT</b> | : | Shenzhen New Huayi Instrument Co., Ltd  |
| <b>ADDRESS</b>   | : | F3, Block 2, Instrument World Industrial Park, Guiyue Road, Longhua New District, Shenzhen City |

|                      |   |   |
|----------------------|---|---|
| <b>MANUFACTURER:</b> | : | Shenzhen New Huayi Instrument Co., Ltd  |
| <b>ADDRESS</b>       | : | F3, Block 2, Instrument World Industrial Park, Guiyue Road, Longhua New District, Shenzhen City |

|                    |   |                      |
|--------------------|---|----------------------|
| <b>SAMPLE TYPE</b> | : | Prototype production |
|--------------------|---|----------------------|



## 2.2 Tested Supporting System Details

| NO. | DESCRIPTION | MANUFACTURER | MODEL | SERIAL NUMBER |
|-----|-------------|--------------|-------|---------------|
| 1.  | -           | N/A          | N/A   | N/A           |

| SIGNAL CABLE DESCRIPTION OF THE ABOVE SUPPORT UNITS |           |       |        |                         |                           |
|---|-----------|-------|--------|-------------------------|---------------------------|
| NO.   | PORT NAME | CABLE | LENGTH | SHIELDED<br>(YES OR NO) | DETACHABLE<br>(YES OR NO) |
| 1   | N/A       | N/A   | N/A    | N/A                     | N/A                       |

## 2.3 Block Diagram of connection between EUT and simulators

**FOR EMI TESTS****FOR EMS TEST**

※ EUT: TEMPERATURE HUMIDITY METER

## 2.4 Test Facility

### 2.4.1 Laboratory Name:

Keyway Testing Technology Co., Ltd.

### 2.4.2 Site Location

Baishun Industrial Zone, Zhangmutou Town, Dongguan, Guangdong, China

### 2.4.3 Test facility:

Certificated by Industry Canada  
 Registration No.: 9868A  
 Date of registration: December 8, 2011

Certificated by FCC, USA  
 Registration No.: 370994  
 Date of registration: January 8, 2015

Certificated by CNAS China  
 Registration No.: CNAS L5783  
 Date of registration: September 13, 2015

## 2.5 Measurement Uncertainty

| Measurement         | Uncertainty |
|---------------------|-------------|
| Conducted emissions | ±2.60dB     |
| Radiated emissions  | ±3.20dB     |

## 2.6 Test Mode Description

| NO. | Test Mode |
|-----|-----------|
| 1   | Running   |


Note: is worst case mode, so is report only reflected the worst mode.

### 3 CONDUCTED DISTURBANCE AT MAINS TERMINALS TEST

#### 3.1 Test Equipment

| Equipment                      | Manufacturer  | Model No. | Serial No. | Last Cal.  | Next Cal.  |
|--------------------------------|---------------|-----------|------------|------------|------------|
| EMI Test Receiver              | Rohde&Schwarz | ESCI      | 101156     | Apr. 27,15 | Apr. 27,16 |
| Artificial Mains Network       | Rohde&Schwarz | ENV216    | 101315     | Apr. 27,15 | Apr. 27,16 |
| Artificial Mains Network (AUX) | Rohde&Schwarz | ENV216    | 101314     | Apr. 27,15 | Apr. 27,16 |
| RF Cable                       | FUJIKURA      | 3D-2W     | 944 Cable  | Apr. 27,15 | Apr. 27,16 |
| Voltage Probe                  | PHX           | A130302   | KWE-053    | Apr. 27,15 | Apr. 27,16 |
| Coupling/Decoupling Network    | FRANKONIA     | A3011081  | KWE-0534   | Apr. 27,15 | Apr. 27,16 |

#### 3.2 Block Diagram of Test Setup

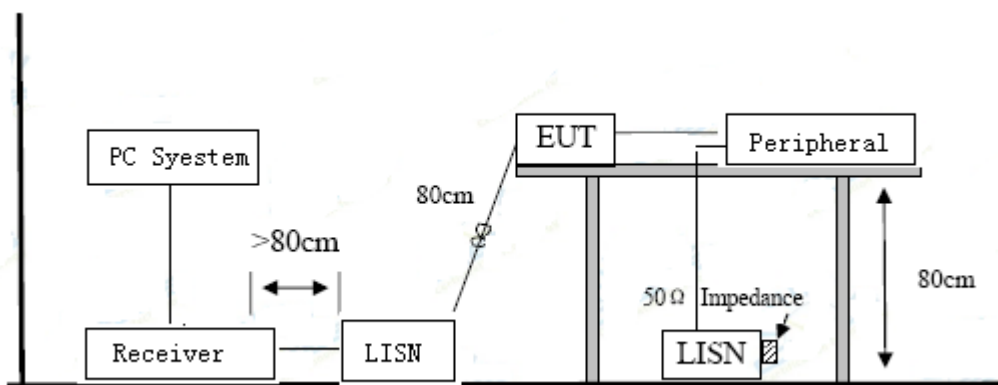

#### 3.3 Test Standard

EN 61326-1: 2013

#### 3.4 Power Line Conducted Disturbance at Mains Terminals Limit

| FREQUENCY       | MAXIMUM RF LINE VOLTAGE |                      |
|-----------------|-------------------------|----------------------|
|                 | Quasi-Peak Level dB(μV) | Average Level dB(μV) |
| 150kHz ~ 500kHz | 66 ~ 56*                | 56 ~ 46*             |
| 500kHz ~ 5MHz   | 56                      | 46                   |
| 5MHz ~ 30MHz    | 60                      | 50                   |

- Notes: 1. Emission level=Read level + LISN factor-Preamp factor + Cable loss  
 2 \* Decreasing linearly with logarithm of frequency.  
 3. The lower limit shall apply at the transition frequencies.

### 3.5 EUT Configuration on Test

The following equipments are installed on Conducted Emission Test to meet EN 61326-1 requirement and operating in a manner which tends to maximize its emission characteristics in a normal application.

#### 3.5.1 Support Equipment :

As Tested Supporting System Detail, In Section 2.2.

### 3.6 Operating Condition of EUT

3.6.1 Setup the EUT and simulator as shown as Section 3.2.

3.6.2 Turn on the power of all equipment.

3.6.3 Let EUT work in test modes and measure it.

### 3.7 Test Procedure

The EUT was placed on a non-metallic table, 80cm above the ground plane. The EUT Power connected to the power mains through a line impedance stabilization network (L.I.S.N. 1#). This provided a 50-ohm coupling impedance for the EUT (Please refer to the block diagram of the test setup and photographs). The other peripheral devices power cord connected to the power mains through a line impedance stabilization network (L.I.S.N.#2). Both sides of power line were checked for maximum conducted interference. In order to find the maximum emission, the relative positions of equipments and all of the interface cables were changed according to EN 61326-1 on conducted Disturbance test.

The bandwidth of test receiver (R & S ESHS20) is set at 10kHz. The frequency range from 150kHz to 30MHz is checked. The test results are reported and test results for Conducted Disturbance Test on Section 3.8.

### 3.8 Conducted Disturbance At Mains Terminals Test Results

EUT Supply By DC Power, So It Not Applicable.

## 4 RADIATED DISTURBANCE TEST

### 4.1 Test Equipments

#### 4.1.1 For Frequency Range 30MHz~1000 MHz (At Semi Anechoic Chamber)


| Equipment                | Manufacturer  | Model No. | Serial No.   | Last Cal.  | Next Cal.  |
|--------------------------|---------------|-----------|--------------|------------|------------|
| EMI Test Receiver        | Rohde&Schwarz | ESCI      | 101156       | Apr. 27,15 | Apr. 27,16 |
| Bilog Antenna            | ETS-LINDGREN  | 3142D     | 00135452     | Apr. 27,15 | Apr. 27,16 |
| Spectrum Analyzer        | Agilent       | 8593E     | 3911A04271   | Apr. 27,15 | Apr. 27,16 |
| 3m Semi-anechoic Chamber | ETS-LINDGREN  | 966       | KW01         | Apr. 27,15 | Apr. 27,16 |
| Signal Amplifier         | SONOMA        | 310       | 187303       | Apr. 27,15 | Apr. 27,16 |
| RF Cable                 | IMRO          | IMRO-400  | 966 Cable 1# | Apr. 27,15 | Apr. 27,16 |
| MULTI-DEVICE Controller  | ETS-LINDGREN  | 2090      | 126913       | N/A        | N/A        |
| Antenna Holder           | ETS-LINDGREN  | 2070B     | 00109601     | N/A        | N/A        |

#### 4.1.2 For Frequency Range 1GHz~6 GHz (At Semi Anechoic Chamber)


| Equipment                | Manufacturer  | Model No. | Serial No.   | Last Cal.  | Next Cal.  |
|--------------------------|---------------|-----------|--------------|------------|------------|
| EMI Test Receiver        | Rohde&Schwarz | ESCI      | 101156       | Apr. 27,15 | Apr. 27,16 |
| Horn Antenna             | DAZE          | ZN30701   | 11003        | Apr. 27,15 | Apr. 27,16 |
| Spectrum Analyzer        | Agilent       | 8593E     | 3911A04271   | Apr. 27,15 | Apr. 27,16 |
| 3m Semi-anechoic Chamber | ETS-LINDGREN  | 966       | KW01         | Apr. 27,15 | Apr. 27,16 |
| Signal Amplifier         | DAZE          | ZN3380C   | 11001        | Apr. 27,15 | Apr. 27,16 |
| RF Cable                 | IMRO          | IMRO-400  | 966 Cable 1# | Apr. 27,15 | Apr. 27,16 |
| MULTI-DEVICE Controller  | ETS-LINDGREN  | 2090      | 126913       | N/A        | N/A        |
| Antenna Holder           | ETS-LINDGREN  | 2070B     | 00109601     | N/A        | N/A        |

### 4.2 Block Diagram Of Test Setup

#### 4.2.1 In Semi Anechoic Chamber (3m) Test Setup Diagram For 30MHz~1000MHz

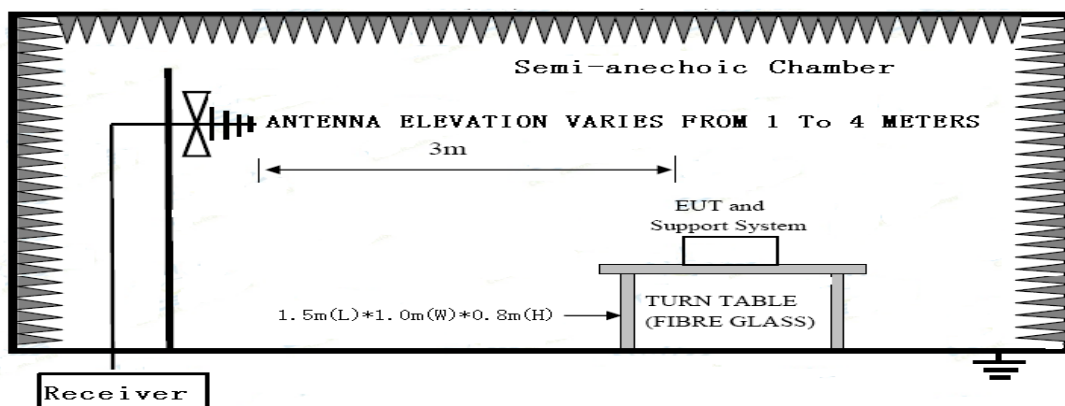

4.2.2 In Semi Anechoic Chamber (3m) Test Setup Diagram for 1-6GHz

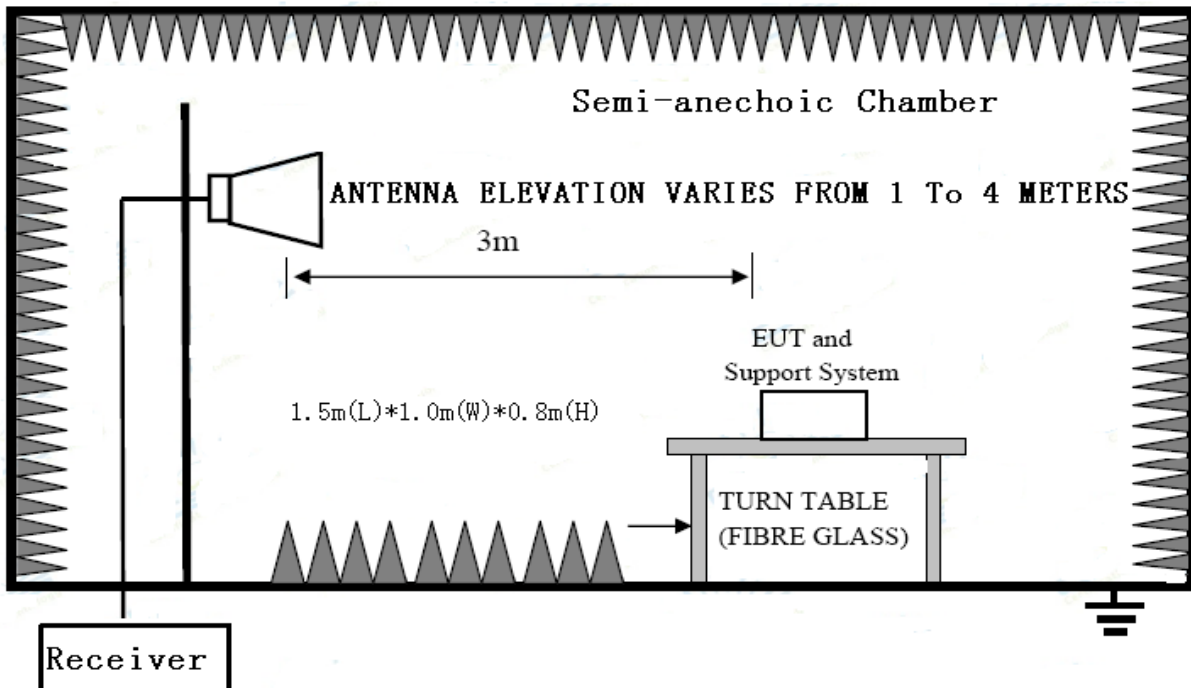

4.3 Test Standard

EN 61326-1: 2013

4.4 Radiated Disturbance Limit

All emanations from a Class B computing devices or system, including any network of conductors and apparatus connected thereto, shall not exceed the level of field strengths specified below:

| FREQUENCY (MHZ) | DISTANCE (Meters) | FIELD STRENGTHS LIMITS (dBµV/m) |
|-----------------|-------------------|---------------------------------|
| 30 ~ 230        | 3                 | 40                              |
| 230 ~ 1000      | 3                 | 70                              |
| 1000~3000       | 3                 | 70(Peak) 50(Average)            |
| 3000~6000       | 3                 | 74(Peak) 54(Average)            |

- Note: (1) Emission level = Read level +Antenna Factor-Preamp Factor +Cable Loss  
 (2) The lower limit shall apply at the transition frequencies.  
 (3) Distance refers to the distance in meters between the test instrument antenna and the closed point of any part of the E.U.T.

#### 4.5 EUT Configuration on Test

The EN 61326-1 Class B regulations test method must be used to find the maximum emission during Radiated Disturbance test. The configuration of EUT is same as used in Conducted Disturbance test. Please refer to Section 3.5.

#### 4.6 Operating Condition of EUT

4.6.1 Setup the EUT and simulator as shown as Section 4.2.

4.6.2 Turned on the power of all equipment

4.6.3 Let EUT work in test modes and measure it.

#### 4.7 Test Procedure

The EUT was placed on a non-metallic table, 80 cm above the ground plane inside a semi-anechoic chamber. An antenna was located 3m & 3m from the EUT on an adjustable mast. A pre-scan was first performed in order to find prominent radiated emissions. For final emissions measurements at each frequency of interest, the EUT were rotated and the antenna height was varied between 1m and 4m in order to maximize the emission. Measurements in both horizontal and vertical polarities were made and the data was recorded. In order to find the maximum emission, the relative positions of equipments and all the interface cables were changed according to EN 61326-1 on Radiated Disturbance test.

The bandwidth setting on the test receiver (ROHDE&SCHWARZ TEST RECEIVER ESCI) is 120 kHz.

The resolution bandwidth of the Agilent Spectrum Analyzer 8593E was set at 1MHz. (For above 1GHz)

The frequency range from 30MHz to 1000MHz was pre-scanned with a peak detector and all final readings of measurement from Test Receiver are Quasi-Peak values.

The frequency range from 1GHz to 6GHz was checked with peak and average detector, measurement distance is 3m in 3m chamber.

Finally, selected operating situations at Semi Anechoic Chamber measurement, all the test results are listed in section 4.8.

#### 4.8 Radiated Disturbance Test Results

### **PASS.**

(All emissions not reported below are too low against the prescribed limits.) The EUT with the following test mode was tested and read QP values, the test results are listed in next pages.

Temperature: 24.4°C Humidity: 54%


The details of test mode is as follows:

| No. | Test Mode |
|-----|-----------|
| 1.  | Running   |

#### FOR FREQUENCY RANGE 1GHz~6GHz

The highest frequency of the internal sources of the EUT is less than 108 MHz, the measurement shall only be made up to 1 GHz. So the frequency rang 1GHz-6GHz radiation test not applicable.




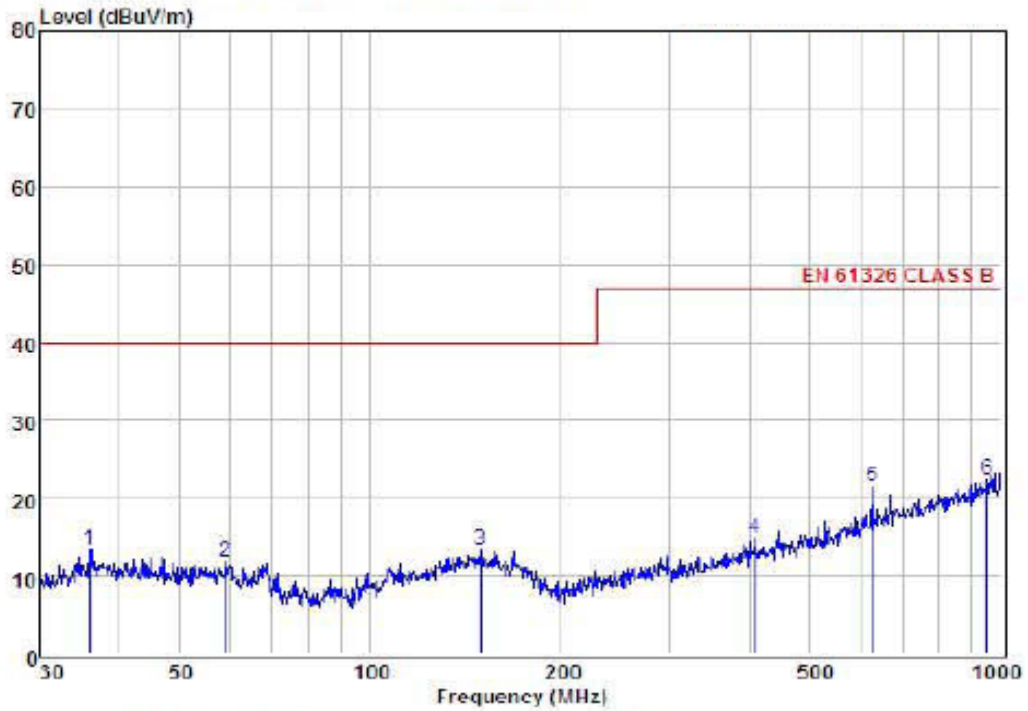

Condition : EN 61326 CLASS B 3m POL: HORIZONTAL  
 EUI : Temperature Humidity Meter  
 Model No : MS6508  
 Test Mode : Running  
 Power : DC 6V  
 Test Engineer : Sky  
 Remark :  
 Temp : 24.2°C  
 Hum : 54%

| Item | Freq<br>MHz | Read<br>Level<br>dBuV | Antenna<br>Factor<br>dB | Preamp<br>Factor<br>dB | Cable<br>Loss<br>dB | Level<br>dBuV | Limit<br>dBuV | Margin<br>dBuV | Remark |
|------|-------------|-----------------------|-------------------------|------------------------|---------------------|---------------|---------------|----------------|--------|
| 1    | 36.00       | 27.37                 | 13.39                   | 27.66                  | 0.11                | 13.21         | 40.00         | -26.79         | QP     |
| 2    | 59.23       | 26.57                 | 12.75                   | 27.87                  | 0.32                | 11.77         | 40.00         | -28.23         | QP     |
| 3    | 150.01      | 25.66                 | 14.16                   | 26.91                  | 0.39                | 13.30         | 40.00         | -26.70         | QP     |
| 4    | 407.51      | 26.40                 | 14.94                   | 27.44                  | 0.83                | 14.63         | 47.00         | -32.17         | QP     |
| 5    | 625.08      | 29.31                 | 18.80                   | 27.82                  | 1.11                | 21.40         | 47.00         | -25.60         | QP     |
| 6    | 948.76      | 26.42                 | 22.13                   | 27.62                  | 1.33                | 22.28         | 47.00         | -24.72         | QP     |

Remark: Level = Read Level + Antenna Factor - Preamp Factor + Cable Loss

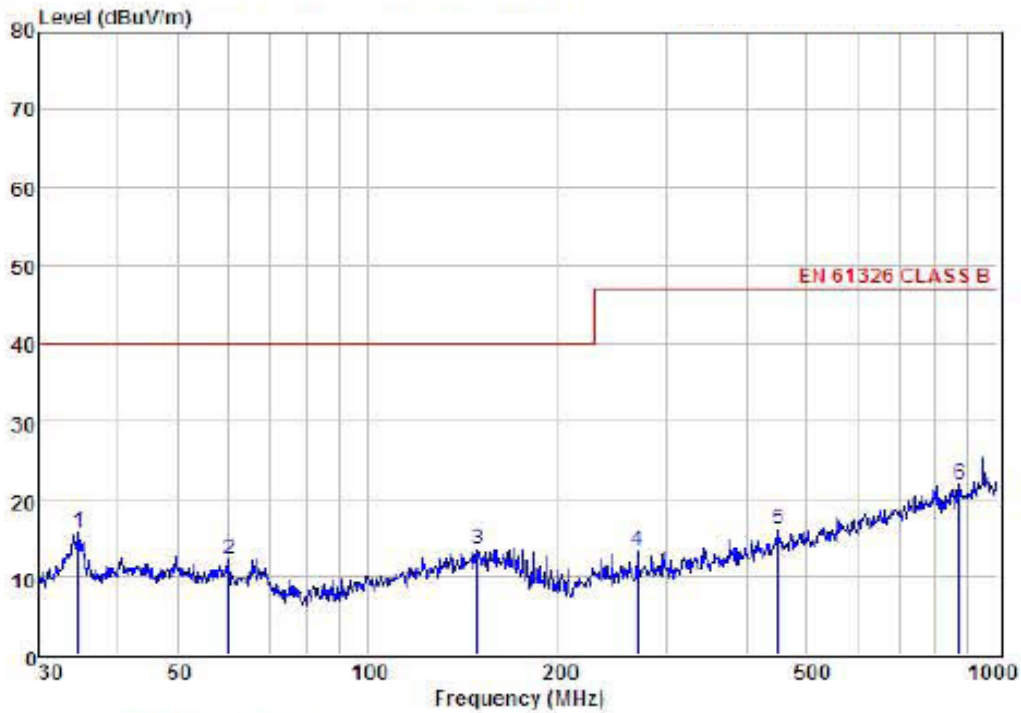

Condition : EN 61326 CLASS B 3m POL: VERTICAL  
 EUT : Temperature Humidity Meter  
 Model No : MS6508  
 Test Mode : Running  
 Power : DC 6V  
 Test Engineer : Sky  
 Remark :  
 Temp : 24.2°C  
 Hum : 54%

| Item | Freq<br>MHz | Read<br>Level<br>dBuV | Antenna<br>Factor<br>dB | Preamplifier<br>Factor<br>dB | Cable<br>Loss<br>dB | Level<br>dBuV | Limit<br>dBuV | Margin<br>dBuV | Remark |
|------|-------------|-----------------------|-------------------------|------------------------------|---------------------|---------------|---------------|----------------|--------|
| 1    | 34.76       | 29.72                 | 13.33                   | 27.58                        | 0.13                | 15.60         | 40.00         | -24.40         | QP     |
| 2    | 60.28       | 27.08                 | 12.75                   | 27.87                        | 0.24                | 12.20         | 40.00         | -27.80         | QP     |
| 3    | 149.49      | 26.01                 | 14.03                   | 26.91                        | 0.35                | 13.48         | 40.00         | -26.52         | QP     |
| 4    | 268.49      | 27.72                 | 12.03                   | 27.14                        | 0.70                | 13.31         | 47.00         | -33.69         | QP     |
| 5    | 449.56      | 26.67                 | 15.97                   | 27.48                        | 1.03                | 16.19         | 47.00         | -30.81         | QP     |
| 6    | 872.18      | 26.93                 | 21.28                   | 27.68                        | 1.38                | 21.91         | 47.00         | -25.09         | QP     |


Remark: Level = Read Level + Antenna Factor - Preamplifier Factor + Cable Loss

## 5 HARMONIC CURRENT TEST

### 5.1 Test Equipments

| Equipment                    | Manufacturer           | Model No.      | Serial No. | Last Cal.  | Next Cal.  |
|------------------------------|------------------------|----------------|------------|------------|------------|
| 5kVA AC Power Source         | California Instruments | 5001iX-CTS-400 | 60138      | Apr. 27,15 | Apr. 27,16 |
| Harmonic/Flicker Test System | California Instruments | PACS-1         | 72847      | Apr. 27,15 | Apr. 27,16 |

### 5.2 Block Diagram of Test Setup

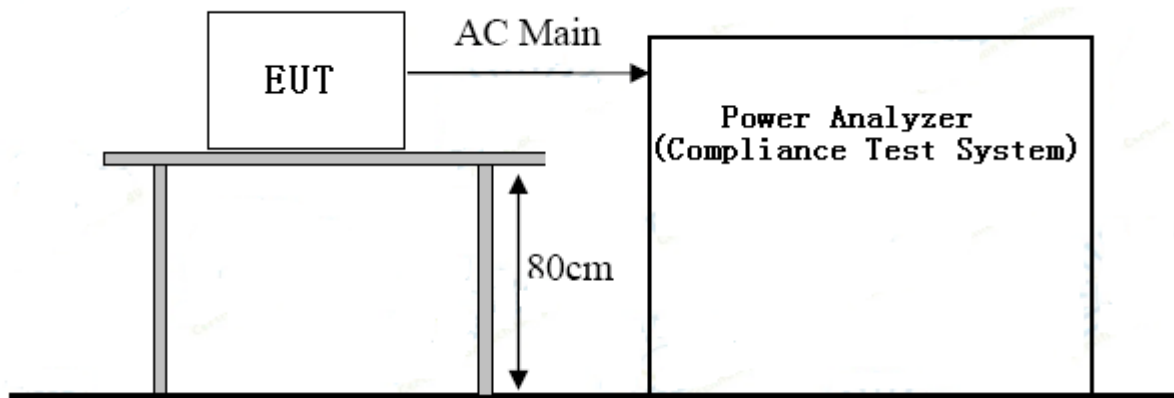

### 5.3 Test Standard

EN 61000-3-2: 2014; Class A

### 5.4 Limits of Harmonic Current

| LIMITS FOR CLASS D EQUIPMENT    |  |  |
|---------------------------------|--|--|
| HARMONIC ORDER (N)              | MAXIMUM PERMISSIBLE HARMONIC CURRENT PER WATT (MA/W) | MAXIMUM PERMISSIBLE HARMONIC CURRENT (A) |
| 3                               | 3.4  | 0.23                                     |
| 5                               | 1.9  | 1.14                                     |
| 7                               | 1.0  | 0.77                                     |
| 9                               | 0.5  | 0.40                                     |
| 11                              | 0.35   | 0.33                                     |
| 13                              | 0.30   | 0.21                                     |
| 15 ≤ n ≤ 39 (odd harmonic only) | 3.85/n   | 0.15 × 15/n                              |

| LIMITS FOR CLASS A EQUIPMENT |   |
|------------------------------|---|
| HARMONIC ORDER<br>N          | MAXIMUM PERMISSIBLE HARMONIC<br>CURRENT A |
| Odd harmonics                |   |
| 3                            | 2,30                                      |
| 5                            | 1,14                                      |
| 7                            | 0,77                                      |
| 9                            | 0,40                                      |
| 11                           | 0,33                                      |
| 13                           | 0,21                                      |
| $15 \leq n \leq 39$          | 0,15 15/n                                 |
| Even harmonics               |   |
| 2                            | 1,08                                      |
| 4                            | 0,43                                      |
| 6                            | 0,30                                      |
| $8 \leq n \leq 40$           | 0,23 8/n                                  |

| LIMITS FOR CLASS A EQUIPMENT            |  |
|---|--|
| HARMONIC ORDER<br>N                     | MAXIMUM PERMISSIBLE HARMONIC<br>CURRENT EXPRESSED AS A<br>PERCENTAGE OF THE INPUT<br>CURRENT AT THE FUNDAMENTAL<br>FREQUENCY % A |
| 2                                       | 2  |
| 3                                       | $30 \cdot \lambda^*$   |
| 5                                       | 10   |
| 7                                       | 7  |
| 9                                       | 5  |
| $11 \leq n \leq 39$                     | 3  |
| (odd harmonics only)                    |  |
| * $\lambda$ is the circuit power factor |  |

### 5.5 Operating Condition of EUT

Same as Section 3.6. except the test setup replaced by Section 5.2.

## 5.6 Test Procedure

The EUT was placed on the top of a wooden table 0.8 meters above the ground and operated to produce the maximum harmonic components under normal operating conditions for each successive harmonic component in turn. The correspondent test program of test instrument to measure the current harmonics emanated from EUT is chosen. The measure time shall be not less than the necessary for the EUT to be exercised

## 5.7 Test Results

EUT Supply by DC Power, So it not applicable.

## 6 VOLTAGE FLUCTUATIONS & FLICKER TEST

### 6.1 Test Equipment

Same as Section 5.1.

### 6.2 Block Diagram of Test Setup

Same as Section 5.2

### 6.3 Test Standard

EN 61000-3-3: 2013

### 6.4 Limits of Voltage Fluctuation and Flick

| TEST ITEM | LIMIT | NOTE   |
|-----------|-------|--|
| Pst       | 1.0   | Pst means Short-term flicker indicator         |
| P1t       | 0.65  | Plt means long-term flicker indicator          |
| P1t       | 0.2   | Tdt means maximum time that dt exceeds 3%      |
| dmax (%)  | 4%    | dmax means maximum relative voltage change.    |
| dc(%)     | 3%    | dc means relative steady-state voltage change. |

### 6.5 Operating Condition of EUT

Same as Section 5.5.

### 6.6 Test Procedure

The EUT was placed on the top of a wooden table 0.8 meters above the ground and operated to produce the most unfavorable sequence of voltage changes under normal conditions. During the flick measurement, the measure time shall include that part of whole operation changes. The observation period for short-term flicker indicator is 10 minutes and the observation period for long-term flicker indicator is 2 hours.

### 6.7 Test Results

EUT Supply by DC Power, So it not applicable.

## 7 IMMUNITY PERFORMANCE CRITERIA

### Performance Level

The test results shall be classified in terms of the loss of function or degradation of performance of the equipment under test, relative to a performance level by its manufacturer or the requestor of the test, or the agreed between the manufacturer and the purchaser of the product.

Definition related to the performance level:

1. Based on the used product standard
2. Based on the declaration of the manufacturer, requestor or purchaser

### Performance criterion A

When seen from the normal viewing distance, the EUT shall operate with no change beyond the manufacturer's specification, in flicker, colour, focus and jitter (except for the power frequency magnetic field test).

### Power frequency magnetic field test

For CRT monitors, the following also applies: The jitter shall be measured using a measuring microscope as specified in 6.6.14 of ISO 9241-3.

$$\frac{(\text{Character height in mm} + 0.3) \times 2.5}{33.3}$$

The jitter (in mm) shall not exceed the value  $\frac{(\text{Character height in mm} + 0.3) \times 2.5}{33.3}$  when the CRT monitor is immersed in a continuous magnetic field of 1A/m (r.m.s.) at one of the power frequencies of 50Hz.

Alternatively, a field of 50A/m may be applied, and a transparent graduated mask used to assess the jitter. In that case, the jitter shall not exceed 50 times the value in the above formula.

NOTE-This test level is used to simplify the measurement of jitter. Lesser values of the test level may be used if non-linearity is experienced, due to, for example, saturation of screening material.

The EUT shall be tested in two positions, both perpendicular to the magnetic field.

### Performance criterion B

Screen disturbances during the application of the test are permissible.

### Performance criterion C


Failures which are not self-recovered after removal of the external disturbance, but which can be recovered to normal operation by reset or reboot are permissible.

## 8 ELECTROSTATIC DISCHARGE IMMUNITY TEST

### 8.1 Test Equipments

| Equipment     | Manufacturer | Model No. | Serial No. | Last Cal.  | Next Cal.  |
|---------------|--------------|-----------|------------|------------|------------|
| ESD Generator | TESEQ        | NSG437    | 433        | Apr. 28,15 | Apr. 28,16 |

### 8.2 Block Diagram of Test Setup

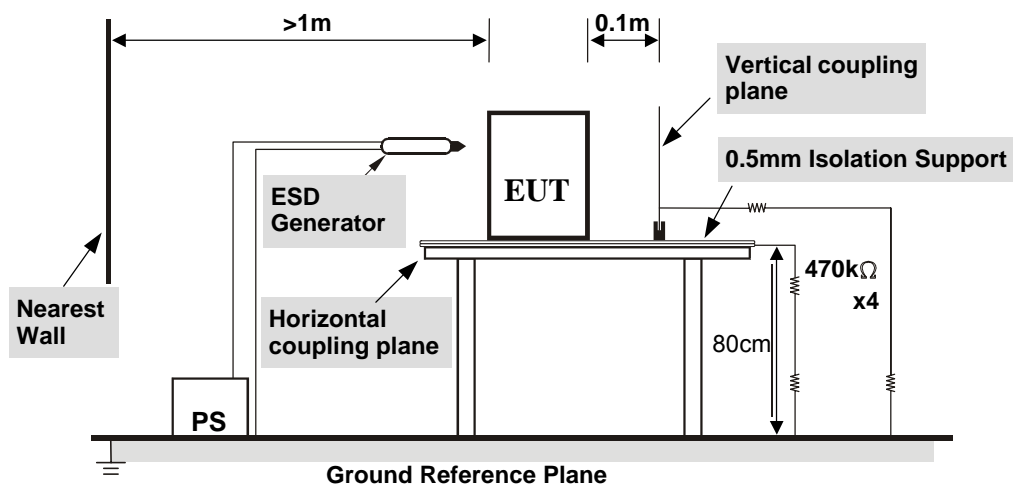

### 8.3 Test Standard

EN 61326-2-2: 2013(IEC 61000-4-2: 2008)  
 (Severity Level 1 & 2 & 3 for Air Discharge at 2 kV & 4 kV & 8kV,  
 Severity Level 1 & 2 for Contact Discharge at 2 kV & 4kV)

### 8.4 Severity Levels and Performance Criterion

#### 8.4.1 Severity level

| LEVEL | TEST VOLTAGE CONTACT DISCHARGE (KV) | TEST VOLTAGE AIR DISCHARGE (KV) |
|-------|-------------------------------------|---------------------------------|
| 1     | 2                                   | 2                               |
| 2     | 4                                   | 4                               |
| 3     | 6                                   | 8                               |
| 4     | 8                                   | 15                              |
| X     | Special                             | Special                         |

#### 8.4.2 Performance criterion : B



## 8.5 EUT Configuration

The configurations of EUT are listed in Section 3.5.

## 8.6 Operating Condition of EUT

Same as Conducted Emission test that is listed in Section 3.6. except the test set up replaced by Section 8.2.

## 8.7 Test Procedure

### 8.7.1 Air Discharge:

The test was applied on non-conductive surfaces of EUT. The round discharge tip of the discharge electrode was approached as fast as possible to touch the EUT. After each discharge, the discharge electrode was removed from the EUT. The generator was re-triggered for a new single discharge and repeated 20 times for each pre-selected test point. This procedure was repeated until all the air discharge completed

### 8.7.2 Contact Discharge:

All the procedure was same as Section 8.7.1. except that the generator was re-triggered for a new single discharge and repeated 50 times for each pre-selected test point. The tip of the discharge electrode was touching the EUT before the discharge switch was operated.

### 8.7.3 Indirect discharge for horizontal coupling plane:

At least 20 single discharges were applied to the horizontal coupling plane, at points on each side of the EUT. The discharge electrode positions vertically at a distance of 0.1m from the EUT and with the discharge electrode touching the coupling plane.

### 8.7.4 Indirect discharge for vertical coupling plane:

At least 20 single discharges were applied to the center of one vertical edge of the coupling plane. The coupling plane, of dimensions 0.5m X 0.5m, was placed parallel to, and positioned at a distance of 0.1m from the EUT. Discharges were applied to the coupling plane, with this plane in sufficient different positions that the four faces of the EUT are completely illuminated.

## 8.8 Test Results

**PASS.**

The EUT was tested and all the test results are listed in next page.

## Electrostatic Discharge Test Results

|                      |  |                    |                  |
|----------------------|--|--------------------|------------------|
| Applicant            | : Shenzhen New Huayi Instrument Co., Ltd | Test Date          | : March 16, 2016 |
| EUT                  | : Temperature Humidity Meter             | Temperature        | : 24°C           |
| M/N                  | : MS6508                                 | Humidity           | : 56%            |
| Test Voltage         | : DC 6V From Battery                     | Test Mode          | : ON             |
| Test Engineer        | : Andy                                   | Pressure           | : 100.6KPa       |
| Required Performance | : B                                      | Actual Performance | : B              |

Air Discharge:  $\pm 2kV \pm 4kV \pm 8kV$  # For Air Discharge each Point Positive 10 times and negative 10 times discharge.  
 Contact Discharge:  $\pm 2kV \pm 4kV$  # For Contact Discharge each point positive 10 times and negative 10 times discharge  
 For the time interval between successive single discharges an initial value of one second.

| Discharge Voltage (kV) | Type of discharge | Dischargeable Points | Performance |             | Result (Pass/Fail) |
|------------------------|-------------------|----------------------|-------------|-------------|--------------------|
|                        |                   |                      | Required    | Observation |                    |
| $\pm 2$                | Air               | 1, 2, 3              | B           | B           | Pass               |
| $\pm 4$                | Air               | 1, 2, 3              | B           | B           | Pass               |
| $\pm 8$                | Air               | 1, 2, 3              | B           | B           | Pass               |
| $\pm 2$                | HCP-Bottom        | Edge of the HCP      | B           | B           | Pass               |
| $\pm 2$                | VCP-Front         | Center of the VCP    | B           | B           | Pass               |
| $\pm 2$                | VCP-Left          | Center of the VCP    | B           | B           | Pass               |
| $\pm 2$                | VCP-Back          | Center of the VCP    | B           | B           | Pass               |
| $\pm 2$                | VCP-Right         | Center of the VCP    | B           | B           | Pass               |
| $\pm 4$                | HCP-Bottom        | Edge of the HCP      | B           | B           | Pass               |
| $\pm 4$                | VCP-Front         | Center of the VCP    | B           | B           | Pass               |
| $\pm 4$                | VCP-Left          | Center of the VCP    | B           | B           | Pass               |
| $\pm 4$                | VCP-Back          | Center of the VCP    | B           | B           | Pass               |
| $\pm 4$                | VCP-Right         | Center of the VCP    | B           | B           | Pass               |

| Discharge Points Description        |            |   |  |
|-------------------------------------|------------|---|--|
| 1                                   | Slots      | 5 |  |
| 2                                   | Button     | 6 |  |
| 3                                   | LED Screen | 7 |  |
| 4                                   |            | 8 |  |
| Test Equipment: ESD Tester (NSG437) |            |   |  |
| Remark:                             |            |   |  |


Discharge was considered on Contact and Air and Horizontal Coupling Plane (HCP) and Vertical Coupling Plane (VCP).

## 9 RF FIELD STRENGTH SUSCEPTIBILITY TEST

### 9.1 Test Equipments

| Equipment         | Manufacturer    | Model No.        | Serial No.           | Last Cal. | Next Cal. |
|-------------------|-----------------|------------------|----------------------|-----------|-----------|
| BiConiLog Antenna | ETS             | 3142C            | 00060445             | Nov.28,15 | Nov.28,16 |
| Amplifier         | BONN ELEKTRONIK | BLWA0840-50/30D  | 066454B              | Nov.28,15 | Nov.28,16 |
| Amplifier         | BONN ELEKTRONIK | BLWA0840-50/100D | 066454A              | Nov.28,15 | Nov.28,16 |
| Signal Generator  | Rohde&Schwarz   | SML03            | 102947               | Nov.28,15 | Nov.28,16 |
| Signal Generator  | Rohde&Schwarz   | SMB100A          | 1406600K02-104532-DF | Nov.28,15 | Nov.28,16 |
| Power Meter       | Rohde&Schwarz   | NRVD             | 102051               | Nov.28,15 | Nov.28,16 |

### 9.2 Block Diagram of Test Setup

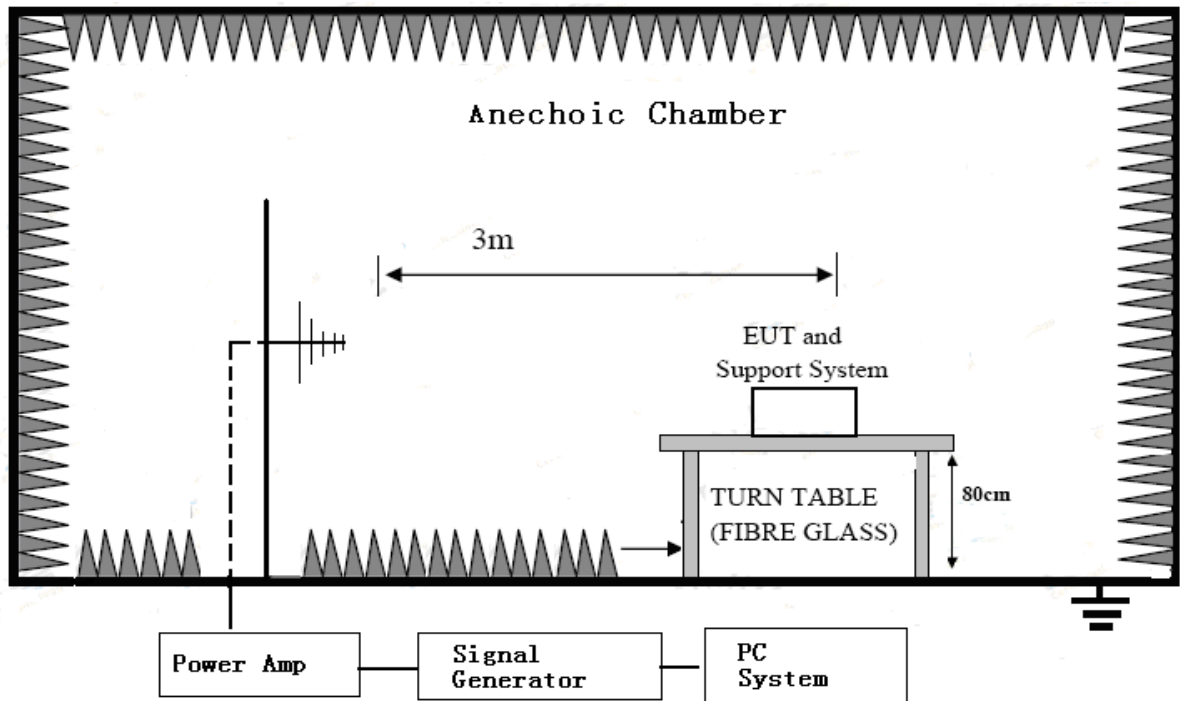

### 9.3 Test Standard

EN 61326-2-2: 2013 (IEC 61000-4-3:2006+A1:2007+A2:2010)  
(Severity Level: 2 at 3V / m)

### 9.4 Severity Levels and Performance Criterion

#### 9.4.1 Limit

| Frequency          | Range  |
|--------------------|--------|
| 80 MHz to 1 GHz    | 10 V/m |
| 1,4 GHz to 2 GHz   | 3 V/m  |
| 2,0 GHz to 2,7 GHz | 1 V/m  |

#### 9.4.2 Severity level

| Level | Test Field Strength V/m |
|-------|-------------------------|
| 1     | 1                       |
| 2     | 3                       |
| 3     | 10                      |
| X     | Special                 |

#### 9.4.3 Performance criterion : A

### 9.5 EUT Configuration

The configurations of EUT are listed in Section 3.5.

### 9.6 Operating Condition of EUT

Same as Conducted Emission test that is listed in Section 3.6. except the test set up replaced by Section 9.2.

## 9.7 Test Procedure

Testing was performed in a Fully anechoic chamber as recommended by IEC 61000-4-3. The EUT was placed on an 80 cm high non-conductive table located in the area of field uniformity. The radiating antenna was placed 3m in front of the EUT and Support system, and dwell time of the radiated interference was controlled by an automated, computer-controlled system. The signal source was stepped through the applicable frequency range at a rate no faster than 1% of the fundamental. The signal was amplitude modulated 80% over the frequency range 80 MHz to 1GHz at a level of 10 V/m, frequency range 1.4 GHz to 2GHz at a level of 3 V/m, frequency range 2 GHz to 2.7GHz at a level of 1 V/m. The dwell time was set at 3 s. Field presence was monitored during testing via a field probe placed in close proximity to the EUT. Throughout testing, the EUT was closely monitored for signs of susceptibility. The test was performed with the antennae oriented in both a horizontal and vertical polarization.

All the scanning conditions are as follows:

| Condition of Test            | Remarks                                       |
|------------------------------|---|
| 1. Test Fielded Strength     | 10 V/m ,3 V/m, 1 V/m                          |
| 2. Radiated Signal           | 80% amplitude modulated with a 1kHz sine wave |
| 3. Scanning Frequency        | 80 - 2700 MHz                                 |
| 4. Sweeping time of radiated | 0.0015 decade/s                               |
| 5. Dwell Time                | 3 Sec.  |

## 9.8 Test Results

### **PASS.**

The EUT was tested and all the test results are listed in next page.

## RF Field Strength Susceptibility Test Results

|   |  |                                 |                  |             |               |
|---|--|---------------------------------|------------------|-------------|---------------|
| Applicant   | : Shenzhen New Huayi Instrument Co., Ltd | Test Date                       | : March 16, 2016 |             |               |
| EUT   | : Temperature Humidity Meter             | Temperature                     | : 24°C           |             |               |
| M/N   | : MS6508                                 | Humidity                        | : 56%            |             |               |
| Test Voltage  | : DC 6V From Battery                     | Test Mode                       | : ON             |             |               |
| Test Engineer   | : Andy                                   | Pressure                        | : 100.6KPa       |             |               |
| Frequency Range   | : 80 MHz -1000MHz                        | Field Strength                  | : 10V/m          |             |               |
| Required Performance  | : A                                      | Actual Performance              | : A              |             |               |
| Modulation: <input checked="" type="checkbox"/> AM <input type="checkbox"/> Pulse <input type="checkbox"/> none    1 kHz 80%  |  |                                 |                  |             |               |
|   |  | Frequency Rang :80 MHz -1000MHz |                  |             |               |
| Steps   | 1%                                       |                                 |                  |             |               |
|   | Horizontal                               |                                 | Vertical         | Result      |               |
|   | Required                                 | Observation                     | Required         | Observation | (Pass / Fail) |
| Front   | A  | A                               | A                | A           | PASS          |
| Right   | A  | A                               | A                | A           | PASS          |
| Rear  | A  | A                               | A                | A           | PASS          |
| Left  | A  | A                               | A                | A           | PASS          |
| Test Equipment : 1. Signal Generator : Rohde&Schwarz    SML03<br>2. Power Amplifier : BONN ELEKTRONIK    BLWA0840-50/30D<br>3. Power Antenna : BONN ELEKTRONIK    BLWA0840-50/30D<br>4. Power Meter : Rohde&Schwarz    NRVD |  |                                 |                  |             |               |
| Remark: No function loss  |  |                                 |                  |             |               |

## RF Field Strength Susceptibility Test Results

|  |  |                                    |                  |             |               |
|--|--|------------------------------------|------------------|-------------|---------------|
| Applicant  | : Shenzhen New Huayi Instrument Co., Ltd | Test Date                          | : March 16, 2016 |             |               |
| EUT  | : Temperature Humidity Meter             | Temperature                        | : 24°C           |             |               |
| M/N  | : MS6508                                 | Humidity                           | : 56%            |             |               |
| Test Voltage   | : DC 6V From Battery                     | Test Mode                          | : ON             |             |               |
| Test Engineer  | : Andy                                   | Pressure                           | : 100.6KPa       |             |               |
| Frequency Range  | : 1400 MHz -2000MHz                      | Field Strength                     | : 3V/m           |             |               |
| Required Performance   | : A                                      | Actual Performance                 | : A              |             |               |
| Modulation: <input checked="" type="checkbox"/> AM <input type="checkbox"/> Pulse <input type="checkbox"/> none    1 kHz    80%  |  |                                    |                  |             |               |
|  |  | Frequency Rang : 1400 MHz -2000MHz |                  |             |               |
| Steps  | 1%                                       |                                    |                  |             |               |
|  | Horizontal                               |                                    | Vertical         | Result      |               |
|  | Required                                 | Observation                        | Required         | Observation | (Pass / Fail) |
| Front  | A  | A                                  | A                | A           | PASS          |
| Right  | A  | A                                  | A                | A           | PASS          |
| Rear   | A  | A                                  | A                | A           | PASS          |
| Left   | A  | A                                  | A                | A           | PASS          |
| Test Equipment : 1. Signal Generator : Rohde&Schwarz    SML03<br>2. Power Amplifier : BONN ELEKTRONIK    BLWA0840-50/30D<br>3. Power Antenna : BONN ELEKTRONIK    BLWA0840-50/30D<br>4. Power Meter :    Rohde&Schwarz    NRVD |  |                                    |                  |             |               |
| Remark: No function loss   |  |                                    |                  |             |               |

## RF Field Strength Susceptibility Test Results

|   |  |                                    |                  |             |               |
|---|--|------------------------------------|------------------|-------------|---------------|
| Applicant   | : Shenzhen New Huayi Instrument Co., Ltd | Test Date                          | : March 16, 2016 |             |               |
| EUT   | : Temperature Humidity Meter             | Temperature                        | : 24°C           |             |               |
| M/N   | : MS6508                                 | Humidity                           | : 56%            |             |               |
| Test Voltage  | : DC 6V From Battery                     | Test Mode                          | : ON             |             |               |
| Test Engineer   | : Andy                                   | Pressure                           | : 100.6KPa       |             |               |
| Frequency Range   | : 2000 MHz -2700MHz                      | Field Strength                     | : 1V/m           |             |               |
| Required Performance  | : A                                      | Actual Performance                 | : A              |             |               |
| Modulation: <input checked="" type="checkbox"/> AM <input type="checkbox"/> Pulse <input type="checkbox"/> none    1 kHz    80%   |  |                                    |                  |             |               |
|   |  | Frequency Rang : 2000 MHz -2700MHz |                  |             |               |
| Steps   | 1%                                       |                                    |                  |             |               |
|   | Horizontal                               |                                    | Vertical         |             | Result        |
|   | Required                                 | Observation                        | Required         | Observation | (Pass / Fail) |
| Front   | A  | A                                  | A                | A           | PASS          |
| Right   | A  | A                                  | A                | A           | PASS          |
| Rear  | A  | A                                  | A                | A           | PASS          |
| Left  | A  | A                                  | A                | A           | PASS          |
| Test Equipment : 1. Signal Generator : Rohde&Schwarz    SML03<br>2. Power Amplifier : BONN ELEKTRONIK    BLWA0840-50/30D<br>3. Power Antenna : BONN ELEKTRONIK    BLWA0840-50/30D<br>4. Power Meter : Rohde&Schwarz    NRVD |  |                                    |                  |             |               |
| Remark: No function loss  |  |                                    |                  |             |               |




## 10 ELECTRICAL FAST TRANSIENT/BURST IMMUNITY TEST

### 10.1 Test Equipments

| Equipment          | Manufacturer | Model No. | Serial No.  | Last Cal. | Next Cal. |
|--------------------|--------------|-----------|-------------|-----------|-----------|
| EFT Tester         | EMtest       | EFT500N5  | V1105108698 | Apr 27,15 | Apr 27,16 |
| EFT Coupling Clamp | EMtest       | HFK       | 0211-168    | Apr 27,15 | Apr 27,16 |

### 10.2 Block Diagram of Test Setup

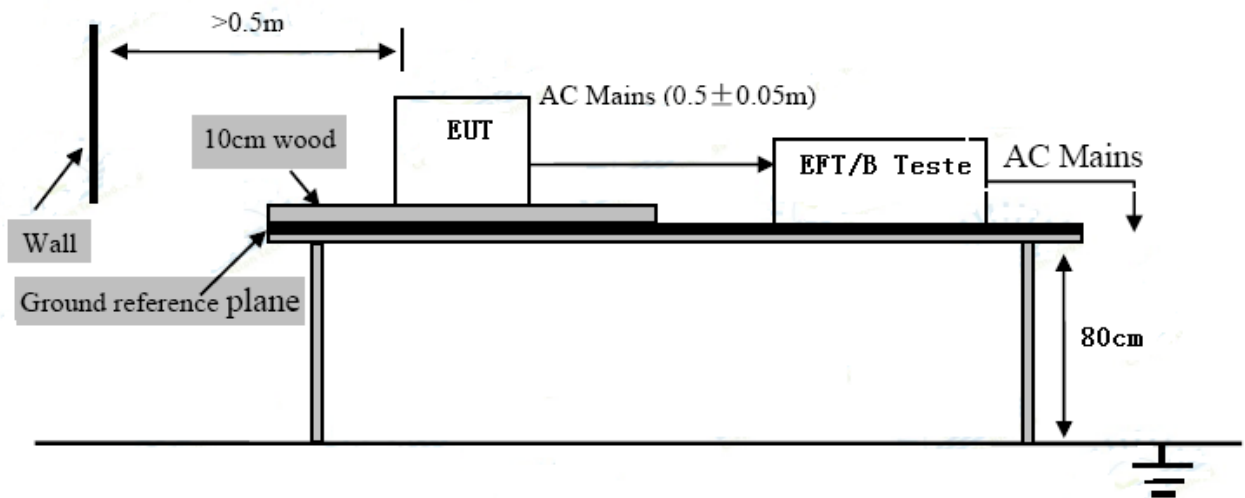

### 10.3 Test Standard

EN 61326-2-2: 2013 (IEC 61000-4-4:2012)  
(Severity Level 2 at 1kV)

### 10.4 Severity Levels and Performance Criterion

#### 10.4.1 Severity level

| Open Circuit Output Test Voltage ±10% |                       |   |
|---------------------------------------|-----------------------|---|
| LEVEL                                 | On Power Supply Lines | On I/O (Input/Output) Signal Data And Control Lines |
| 1                                     | 0.5 kV                | 0.25 kV   |
| 2                                     | 1 kV                  | 0.5 kV  |
| 3                                     | 2 kV                  | 1 kV  |
| 4                                     | 4 kV                  | 2 kV  |
| X                                     | Special               | Special   |

#### 10.4.2 Performance criterion : B

## 10.5 EUT Configuration

The configurations of EUT are listed in Section 3.5.

## 10.6 Operating Condition of EUT

Same as Conducted Emission test that is listed in Section 3.6. except the test set up replaced by Section 10.2.

## 10.7 Test Procedure

The EUT and its simulators were placed on the ground reference plane and were insulated from it by a wood support 0.1m + 0.01m thick. The ground reference plane was 1m\*1m metallic sheet with 0.65mm minimum thickness. This reference ground plane was project beyond the EUT by at least 0.1m on all sides and the minimum distance between EUT and all other conductive structure, except the ground plane was more than 0.5m. All cables to the EUT was placed on the wood support, cables not subject to EFT/B was routed as far as possible from the cable under test to minimize the coupling between the cables.

### 10.7.1 For input and AC power ports:

The EUT was connected to the power mains by using a coupling device that couples the EFT interference signal to AC power lines. Both positive transients and negative transients of test voltage were applied during compliance test and the duration of the test can't less than 1min.

### 10.7.2 For signal lines and control lines ports:

It's unnecessary to test.

### 10.7.3 For DC input and DC output power ports:

It's unnecessary to test.

## 10.8 Test Results


EUT Supply by DC Power, So it not applicable.

## 11 SURGE TEST

### 11.1 Test Equipments

| Equipment                       | Manufacturer | Model No.     | Serial No.  | Last Cal.  | Next Cal.  |
|---------------------------------|--------------|---------------|-------------|------------|------------|
| Surge Tester                    | EMtest       | UCS500N7      | V1105108699 | Apr. 27,15 | Apr. 27,16 |
| EMS Multifunctional test system | SCHAFFNER    | 6100Series    | 34326       | Apr. 27,15 | Apr. 27,16 |
| Transient Immunity test system  | EMC-PARTNER  | TRANSIENT2000 | 845         | Apr. 27,15 | Apr. 27,16 |

### 11.2 Block Diagram of Test Setup

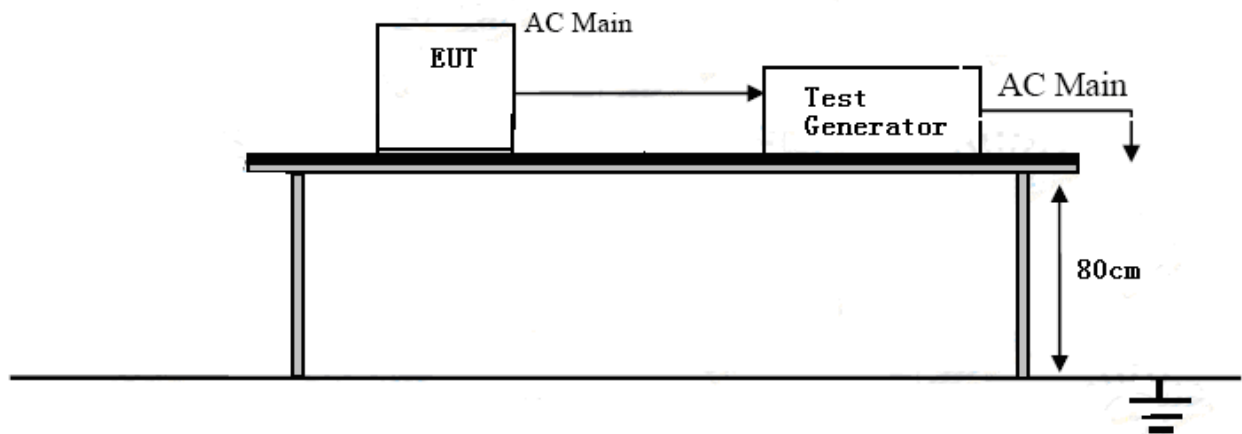

### 11.3 Test Standard

EN 61326-2-2: 2013 (IEC 61000-4-5: 2014)  
 (Severity Level: Line to Line was Level 2 at 1kV)

### 11.4 Severity Levels and Performance Criterion

#### 11.4.1 Severity level

| SEVERITY LEVEL | OPEN-CIRCUIT TEST VOLTAGE KV |
|----------------|------------------------------|
| 1              | 0.5                          |
| 2              | 1.0                          |
| 3              | 2.0                          |
| 4              | 4.0                          |
| *              | SPECIAL                      |

#### 11.4.2 Performance criterion: B

## 11.5 EUT Configuration

The configurations of EUT are listed in Section 3.5.

## 11.6 Operating Condition of EUT

Same as Conducted Emission test that is listed in Section 3.6. except the test set up replaced by Section 11.2

## 11.7 Test Procedure

- 1) Set up the EUT and test generator as shown on Section 11.2.
- 2) For line-to-line coupling mode, provide a 1kV 1.2/50us voltage surge (at open-circuit condition) and 8/20us current surge to EUT selected points, and for active line / neutral lines to ground are same except test level is 2kV.
- 3) At least 5 positive and 5 negative (polarity) tests with a maximum 1/min repetition rate are applied during test.
- 4) Different phase angles are done individually.
- 5) Record the EUT operating situation during compliance test and decide the EUT immunity criterion for above each test.

## 11.8 Test Results

EUT Supply by DC Power, So it not applicable.


## 12 INJECTED CURRENTS SUSCEPTIBILITY TEST

### 12.1 Test Equipments

| Equipment                       | Manufacturer | Model No.   | Serial No. | Last Cal.  | Next Cal.  |
|---------------------------------|--------------|-------------|------------|------------|------------|
| C/S Test System                 | EMtest       | CIT-10      | 126B1164   | Apr. 27,15 | Apr. 27,16 |
| CDN                             | Luthi        | L-801 M2/M3 | 2789       | Apr. 27,15 | Apr. 27,16 |
| Electromagnetic Injection Clamp | Luthi        | EM101       | 36041      | Apr. 28,15 | Apr. 28,16 |

### 12.2 Block Diagram of Test Setup

50 Ω TERMINATOR

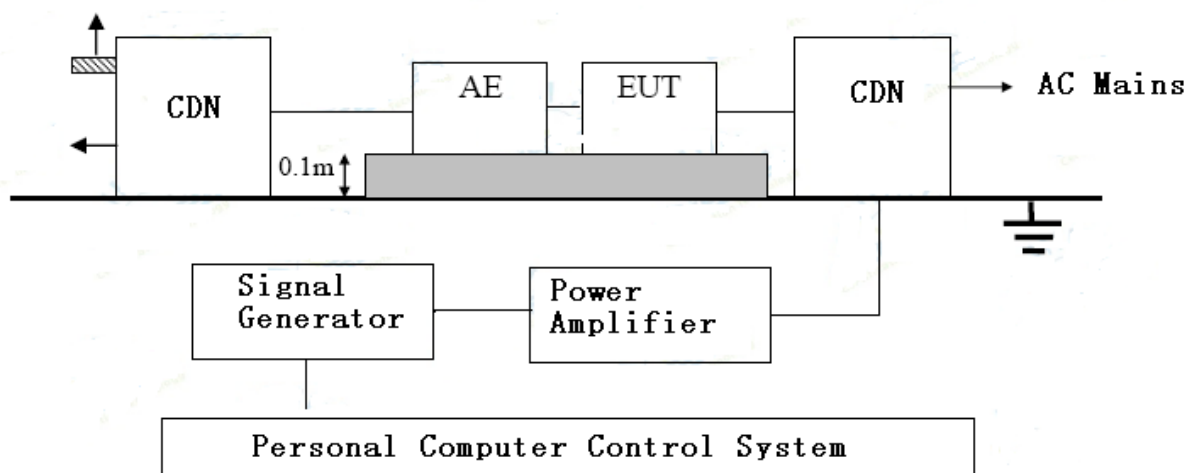

### 12.3 Test Standard

EN 61326-2-2: 2013 (IEC 61000-4-6: 2013) (Severity Level 2 at 3V (r.m.s.) and frequency is from 0.15MHz to 80MHz)

### 12.4 Severity Levels and Performance Criterion

#### 12.4.1 Severity level

| LEVEL | VOLTAGE LEVEL (E.M.F.) V |
|-------|--------------------------|
| 1     | 1                        |
| 2     | 3                        |
| 3     | 10                       |
| *     | SPECIAL                  |

#### 12.4.2 Performance criterion: A

## 12.5 EUT Configuration

The configurations of EUT are listed in Section 3.5.

## 12.6 Operating Condition of EUT

Same as Conducted Emission test that is listed in Section 3.6. except the test set up replaced by Section 12.2.

## 12.7 Test Procedure

- 1) Set up the EUT, CDN and test generators as shown on Section 12.2.
- 2) Let the EUT work in test mode and test it.
- 3) The EUT are placed on an insulating support 0.1m high above a ground reference plane. CDN (coupling and decoupling device) is placed on the ground plane about 0.3m from EUT. Cables between CDN and EUT are as short as possible, and their height above the ground reference plane shall be between 10 and 30 mm (where possible).
- 4) The disturbance signal described below is injected to EUT through CDN.
- 5) The EUT operates within its operational mode(s) under intended climatic conditions after power on.
- 6) The frequency range is swept from 0.150MHz to 80MHz using 3V signal level, and with the disturbance signal 80% amplitude modulated with a 1kHz sine wave.
- 7) The rate of sweep shall not exceed  $1.5 \times 10^{-3}$  decades/s. Where the frequency is swept incrementally, the step size shall not exceed 1% of the start and thereafter 1% of the preceding frequency value.
- 8) Recording the EUT operating situation during compliance testing and decide the EUT immunity criterion.

## 12.8 Test Results


EUT Supply by DC Power, So it not applicable.

### 13 MAGNETIC FIELD IMMUNITY TEST

#### 13.1 Test Equipments

| Equipment                | Manufacturer | Model No.   | Serial No.        | Last Cal. | Next Cal. |
|--------------------------|--------------|-------------|-------------------|-----------|-----------|
| Magnetic Field Generator | EVERFINE     | EMS61000-8K | YG100376N11080002 | Apr 27,15 | Apr 27,16 |

#### 13.2 Block Diagram of Test Setup

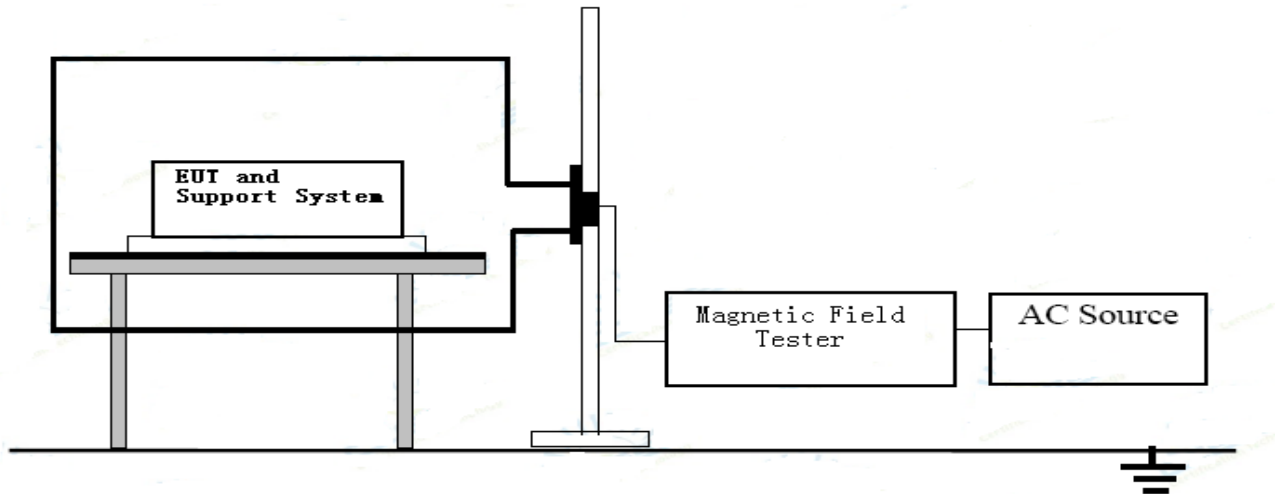

#### 13.3 Test Standard

EN 61326-2-2: 2013 (IEC 61000-4-8: 2009)  
(Severity Level 1 at 1A/m)

#### 13.4 Severity Levels and Performance Criterion

##### 13.4.1 Severity level

| LEVEL | MAGNETIC FIELD STRENGTH A/M |
|-------|-----------------------------|
| 1     | 1                           |
| 2     | 3                           |
| 3     | 10                          |
| 4     | 30                          |
| 5     | 100                         |
| X     | SPECIAL                     |

##### 13.4.2 Performance criterion : A

### 13.5 EUT Configuration on Test

The configurations of EUT are listed in Section 3.5.

### 13.6 Operating Condition of EUT

Same as Conducted Emission test that is listed in Section 3.6. except the test set up replaced by Section 13.2.

### 13.7 Test Procedure

The EUT was subjected to the test magnetic field by using the induction coil of standard dimensions (1m\*1m) and shown in Section 13.2. The induction coil was then rotated by 90° in order to expose the EUT to the test field with different orientations.

### 13.8 Test Results

**PASS.**

The EUT was tested and all the test results are listed in next page.



## Magnetic Field Immunity Test Results


| Applicant  | :                | Shenzhen New Huayi Instrument Co., Ltd | Test Date          | :           | March 16, 2016 |
|--|------------------|--|--------------------|-------------|----------------|
| EUT  | :                | Temperature Humidity Meter             | Temperature        | :           | 24°C           |
| M/N  | :                | MS6508                                 | Humidity           | :           | 56%            |
| Test Voltage   | :                | DC 6V From Battery                     | Test Mode          | :           | ON             |
| Test Engineer  | :                | Andy                                   | Pressure           | :           | 100.6KPa       |
| Required Performance   | :                | A                                      | Actual Performance | :           | A              |
| Test Level   | Testing Duration | Coil Orientation                       | Required           | Observation | RESULT         |
|  |                  |  |                    |             | (Pass /Fail)   |
| 1A/m   | 5 min / coil     | X                                      | A                  | A           | PASS           |
| 1A/m   | 5 min / coil     | Y                                      | A                  | A           | PASS           |
| 1A/m   | 5 min / coil     | Z                                      | A                  | A           | PASS           |
| Test Equipment :Magnetic Field Tester (EMS61000-8K)  |                  |  |                    |             |                |
| Remark1: The products not have magnetically sensitive equipment.<br>Remark2: No function loss. |                  |  |                    |             |                |

## 14 VOLTAGE DIPS AND INTERRUPTIONS TEST

### 14.1 Test Equipment

| Equipment   | Manufacturer | Model No.    | Serial No.            | Last Cal. | Next Cal. |
|-------------|--------------|--------------|-----------------------|-----------|-----------|
| Dips Tester | EVERFINE     | EMS61000-11K | YG100319N1104<br>0005 | Apr 27,15 | Apr 27,16 |

### 14.2 Block Diagram of Test Setup

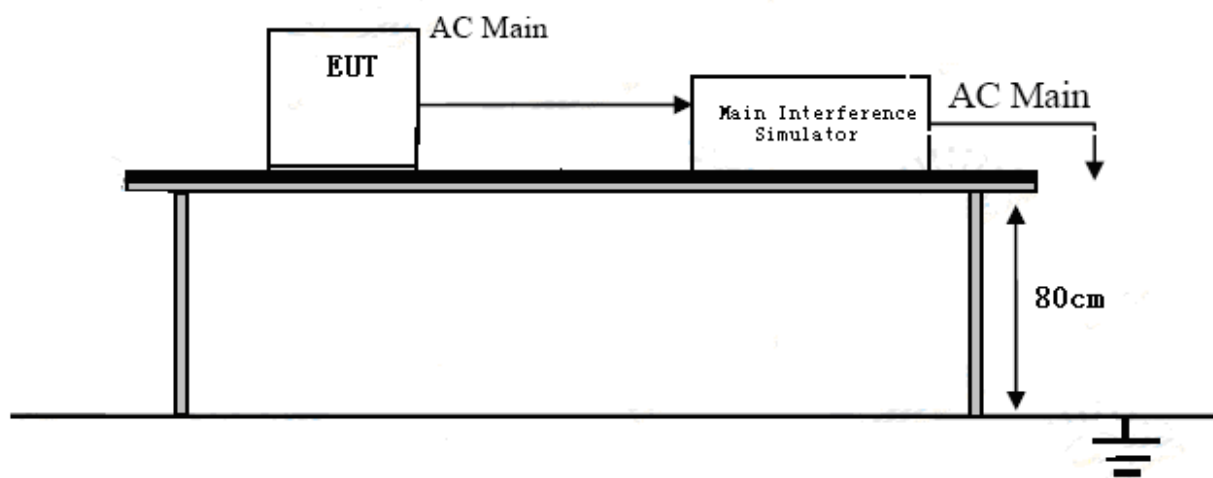

### 14.3 Test Standard

EN 61326-2-2: 2013(IEC 61000-4-11:2004)

### 14.4 Severity Levels and Performance Criterion

#### 14.4.1 Severity level

| TEST LEVEL %UT | VOLTAGE DIP AND SHORT INTERRUPTIONS% UT | PERFORMANCE CRITERION | DURATION (IN PERIOD) |
|----------------|---|-----------------------|----------------------|
| 0              | 100                                     | C                     | 250                  |
| 0              | 100                                     | B                     | 0.5                  |
| 70             | 30                                      | C                     | 25                   |

#### 14.4.2 Performance criterion : B & C

#### 14.5 EUT Configuration

The configurations of EUT are listed in Section 3.5.

#### 14.6 Operating Condition of EUT

Same as Conducted Emission test that is listed in Section 3.6. except the test set up replaced by Section 14.2.

#### 14.7 Test Procedure



- 1) The EUT and test generator were setup as shown on Section 14.2.
- 2) The interruption is introduced at selected phase angles with specified duration.
- 3) Record any degradation of performance.

#### 14.8 Test Results

EUT Supply by DC Power, So it not applicable.

## 15 PHOTOGRAPHS OF THE TEST CONFIGURATION

### 15.1 Photos of Radiated Emission Test (In Anechoic Chamber)

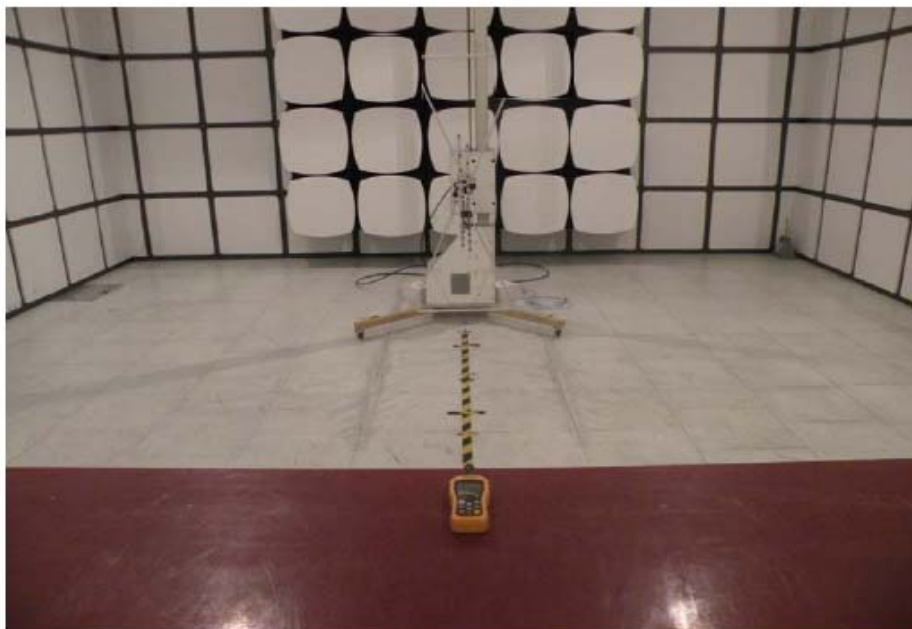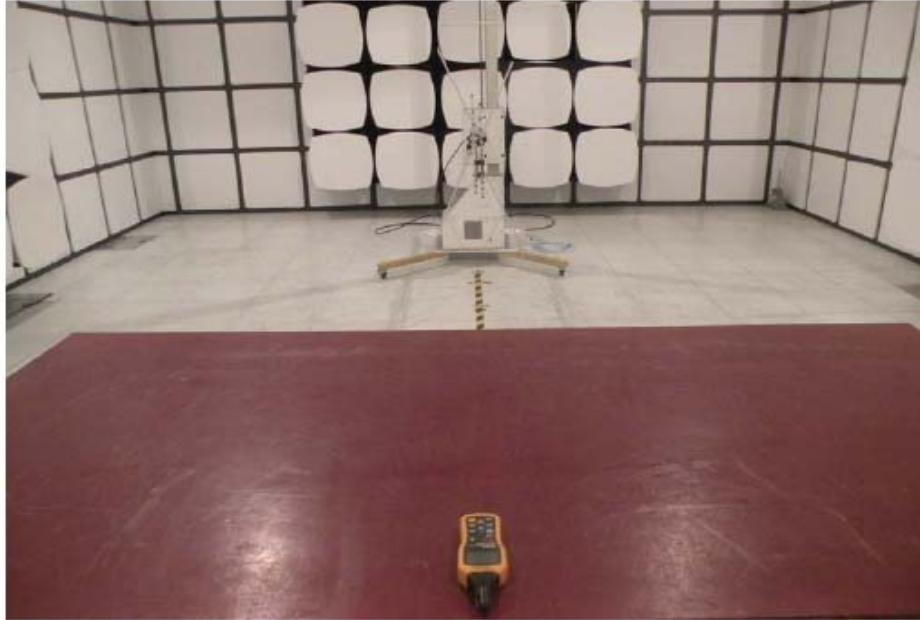

## 15.2 Photos of Electrostatic Discharge Immunity Test



**16 PHOTOS OF THE EUT**

**Photo 1# Unit overview**



**Photo 2# Unit Overview**



**Photo 3# Unit Overview**



**Photo 4# Unit Overview**





**Photo 5# Internal View**



**Photo 6# Internal View**





**Photo 7# Internal View**

